Intensive Care Med
https://doi.org/10.1007/s00134-026-08420-7

NARRATIVE REVIEW

Non-invasive intracranial pressure estimation in the intensive care unit: narrative review of methods and clinical applications

Edoardo Picetti[1], Daniele Guerino Biasucci[2], Elisa Gouvea Bogossian[3], Sérgio Brasil[4], Danilo Cardim[5,6], Marek Czosnyka[7], Daniel A. Godoy[8], Gregory W. J. Hawryluk[9], Mohammad I. Hirzallah[10,11], Frank A. Rasulo[12,13], Carla Bittencourt Rynkowski[14,15], Andres M. Rubiano[8], Fabio Silvio Taccone[3] and Chiara Robba[16*]

© 2026 The Author(s)

Abstract: Despite invasive methods are the gold standard for intracranial pressure (ICP) measurement, several non-invasive techniques (nICP) have been proposed as surrogate, although their use remains insufficiently recognized in clinical practice. These include transcranial Doppler blood flow velocity assessment (arterial or venous), optic nerve sheath diameter (ONSD), automated pupillometry, measurement of skull expansion and compliance, brain imaging, double-depth ophthalmic artery blood flow velocity, and ultrasound time-of-flight. The main limitations of all indirect methods are calibration and zeroing, which constrain the absolute accuracy of non-invasive ICP monitoring. For transcranial Doppler-based methods, the 95% limits of agreement are approximately ± 7–15 mmHg, while for ONSD-based techniques they range from ± 7–10 mmHg. Improved predictive accuracy may be achieved by combining different modalities and applying advanced signal analysis techniques. Importantly, in patients with acute brain injury, nICP can complement invasive monitoring by guiding patient selection for urgent monitoring, facilitating brain assessment in moderate traumatic brain injury, and assisting management in patients with coagulopathy. In the general intensive care population, nICP may provide valuable information after cardiac arrest, liver failure, and sepsis. In the emergency department, early detection of intracranial hypertension helps prevent missing the "golden hour" of brain care. Finally, nICP is particularly relevant in low-resource settings, where intensive care facilities are limited.

*Correspondence: kiarobba@gmail.com
[16] IRCCS, Policlínico San Martino, Genoa, Italy
Full author information is available at the end of the article

Springer

SHOUT
SHARE
IT

Graphical abstract:

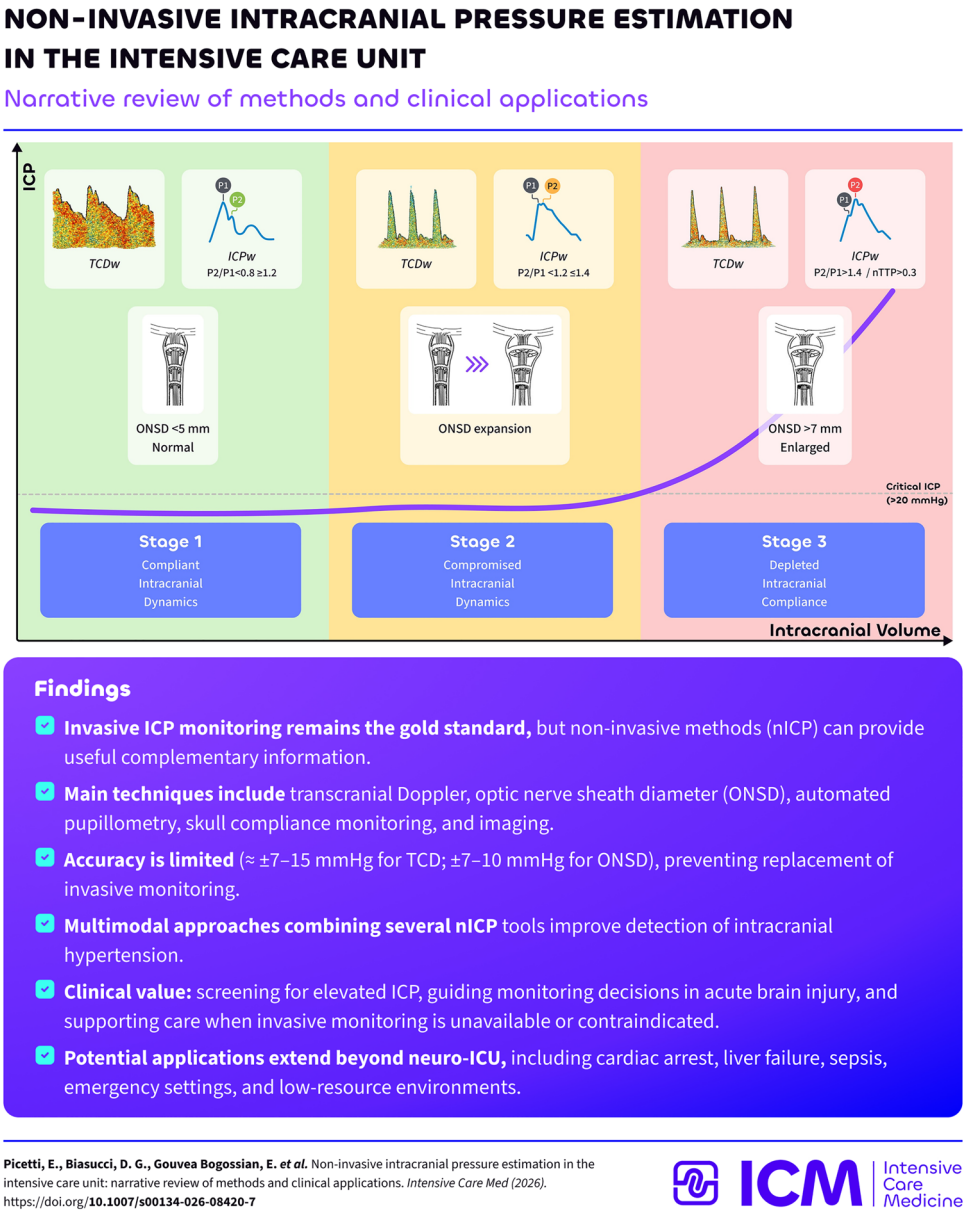
NON-INVASIVE INTRACRANIAL PRESSURE ESTIMATION
IN THE INTENSIVE CARE UNIT
Narrative review of methods and clinical applications
ICP
TCDw
ICPw
P2/P1<0.8 ≥1.2
TCDw
ICPw
P2/P1 <1.2 ≤1.4
TCDw
ICPw
P2/P1>1.4 / nTTP>0.3
ONSD <5 mm
Normal
ONSD expansion
ONSD >7 mm
Enlarged
Critical ICP
(>20 mmHg)
Stage 1
Compliant
Intracranial
Dynamics
Stage 2
Compromised
Intracranial
Dynamics
Stage 3
Depleted
Intracranial
Compliance
Intracranial Volume
Findings
Invasive ICP monitoring remains the gold standard, but non-invasive methods (nICP) can provide useful complementary information.
Main techniques include transcranial Doppler, optic nerve sheath diameter (ONSD), automated pupillometry, skull compliance monitoring, and imaging.
Accuracy is limited (≈ ±7–15 mmHg for TCD; ±7–10 mmHg for ONSD), preventing replacement of invasive monitoring.
Multimodal approaches combining several nICP tools improve detection of intracranial hypertension.
Clinical value: screening for elevated ICP, guiding monitoring decisions in acute brain injury, and supporting care when invasive monitoring is unavailable or contraindicated.
Potential applications extend beyond neuro-ICU, including cardiac arrest, liver failure, sepsis, emergency settings, and low-resource environments.
Picetti, E., Biasucci, D. G., Gouvea Bogossian, E. et al. Non-invasive intracranial pressure estimation in the intensive care unit: narrative review of methods and clinical applications. Intensive Care Med (2026).
https://doi.org/10.1007/s00134-026-08420-7
ICM Intensive Care Medicine

Keywords: Non-invasive intracranial pressure, Outcome, Intensive care medicine, Secondary brain damage, Brain ultrasound, Automated pupillometry

Introduction

Intracranial hypertension (IH) after acute brain injury (ABI) is an important cause of secondary brain damage and remains a matter of continuous investigation [1]. It is widely recognized that intracranial pressure (ICP) is 'more than the number'; therefore, its continuous monitoring should be considered as a mandatory tool to avoid additional brain insults, resulting from a hyperdynamic course of ICP (plateau waves, sudden refractory hypertension, changes in arterial partial pressure of carbon dioxide ($PaCO_2$), etc.) [1]. Despite the lack of a positive Level-I evidence on outcome in traumatic brain injury (TBI), ICP monitoring is generally considered of paramount importance in the neuro-intensive care setting [2–5]. Invasive methods

(i.e., intraparenchymal and external ventricular drain (EVD) systems) are considered the gold standard for ICP measurement and treatment [6]. However, in some settings (e.g., low-income countries, austere environments, etc.), these systems are not immediately and easily available. Moreover, patients may have contraindications for invasive tools (i.e., infections, coagulopathy) or may not completely meet indications for insertion. This has induced many authors to focus their efforts, over the last decades, on the study of non-invasive ICP (nICP) estimators [7, 8]. A variety of non-invasive tools have been proposed, each with different levels of accuracy, availability, and feasibility (Table 1) [8]. Although none of these modalities has demonstrated sufficient accuracy to replace invasive ICP monitoring (mainly due to lack of calibration and zeroing), several have shown potential to complement invasive measurements. Rather than serving as substitutes, non-invasive tools provide additional, clinically relevant information regarding the risk and likelihood of IH. Importantly, they may also add value even when invasive ICP monitoring is in place, by contributing complementary physiological insights that support clinical decision-making across a range of settings [9]. Importantly, high sensitivity and high specificity are generally mutually exclusive. For example, a highly sensitive approach will result in many patients undergoing invasive monitoring unnecessarily, whereas a highly specific strategy risks missing patients with elevated ICP. This review aims to provide clinicians involved in the care of critical care patients [e.g., emergency physicians, general intensive care unit (ICU) physicians, neurosurgeons, etc.] with an updated overview on the methodology and clinical applications of nICP monitoring tools.

Take-home message

Although invasive intracranial pressure (ICP) monitoring tools remain the gold standard for diagnosing and managing intracranial hypertension, non-invasive methods (nICP) can provide valuable support in specific conditions.

Each nICP method has specific own strengths, methodological limitations and variable accuracy; therefore, a combination of different complementary tools is warranted to raise or exclude the suspicion of intracranial hypertension.

Methods for non-invasive ICP estimation

Transcranial Doppler: pulsatility index and diastolic flow velocity formula

Transcranial Doppler (TCD) ultrasound offers a portable, bedside method to measure cerebral blood flow (CBF) velocities in basal intracranial arteries, most commonly the middle cerebral artery (MCA). Because ICP alters intracranial compliance and distal cerebrovascular resistance, mainly due to changes in cerebral perfusion pressure (CPP), TCD waveform variations, especially in diastolic flow and pulsatility, have been studied extensively as non-invasive surrogates to estimate ICP and CPP in critically ill patients (Fig. 1). The cranial vault is a fixed-volume compartment in which arterial inflow, venous outflow, cerebrospinal fluid (CSF) and brain tissue volume interact, resulting in modulation of ICP. An increase in ICP reduces CPP, decreasing downstream vascular resistance (in patients with intact autoregulation mechanism) and increases critical closing pressure (CrCP), and preferentially diminishes diastolic flow. These hemodynamic changes modify the shape of the arterial velocity waveform recorded by TCD; systolic peaks may be preserved or even slightly increased, while end-diastolic velocities (EDV or FVd) fall, producing greater waveform pulsatility that can be quantified by the pulsatility index (PI) [10]. As TCD records peak systolic velocity (PSV), EDV, and time-averaged mean velocity (MV or FVm) from basal cerebral arteries, PI is calculated as (PSV − EDV)/MV. The PI mathematically can be described as a complex function of CPP, arterial blood pulse pressure, cerebrovascular resistance, compliance, and heart rate [11]. Therefore, PI is modulated by systemic hemodynamics (acute mean arterial pressure (MAP) changes, heart rate), arterial properties (stiffness, atherosclerosis), ventilatory status ($PaCO_2$), vasoactive drugs, and operator/acoustic window variability. These confounders can change PI independently of true CPP and ICP. For example, in case of vasospasm, PI may be altered by arterial narrowing rather than IH. As such, multivariable regression and machine-learning models that combine continuous waveform features with systemic inputs [MAP, $PaCO_2$/end-tidal CO_2 ($ETCO_2$), heart rate] and patient factors (age, vascular comorbidity) may improve classification of elevated ICP and sensitivity to therapeutic responses [12]. The TCD-PI presents a sensitivity and specificity of 0.74 for an optimal cut-off value of 1.28 [9] (ESM 1). Another quantitative nICP estimation from TCD can be performed using empirical formulas combining systemic arterial pressure with Doppler flow velocities. A commonly applied two-step method [13, 14] estimates non-invasive CPP (nCPP) from the ratio of FVd to FVm, then derives nICP from MAP:

$$nCPP = MAP \times \left(\frac{FVd}{FVm}\right) + 14$$

$$nICP = MAP - nCPP.$$

Table 1 Summary of different commercially available bedside non-invasive ICP methods with pros, cons availability, limitations, costs

Technique	Principle	Cut-offs for IH/ IH indicators and sensitivity/specificity	Pros	Cons	Commercial information[a]	
Automated pupillometry	Quantifies pupillary parameters, such as size, constriction and dilation velocities, and light response latency	NPi ≤ 3 suggests brainstem injury, possibly due to cerebral herniation Sensitivity = 0.68 and specificity = 0.68 for an optimal cut-off value of 3.96 [ESM 1]	Eliminates the subjectivity and inter-observer variability inherent in manual pupillary assessment. The Neurologic Pupillary index -NPi- provides an objective and aggregated score that has shown a strong correlation with outcomes in acute brain injury patients	Pupillometry may not detect more subtle or early ICP changes The exact cause of pupillary abnormalities (direct nerve injury versus ICP-related compression versus medication effect) still requires comprehensive clinical evaluation and can be challenging in cases of polytrauma or complex neurological conditions	Several providers. (NPi is a proprietary parameter from a single provider)	Low cost but disposable lens are intended for limited scans; not restricted to use by a specific professional
Optic nerve sheath diameter ultrasound	Ultrasound can assess the optic nerve sheath, which expands with increased ICP	Nerve sheath ≥ 6 mm indicates IH Sensitivity = 0.83 and specificity = 0.83 regarding an optimal cut-off value of 5.9 mm [ESM1]	This procedure can be carried out by both nurses and physicians. It requires training to achieve competency	Serial monitoring is employed. The literature reports different cutoffs and approaches to assess intracranial hypertension. The effects of clinical interventions remain to be established	Several providers	One-time device purchase. No disposables
Skull microdeformation	ICP waveforms can be reproduced from micrometric detection of skull pulsation synchronized with each heartbeat	P2/P1 ratio ≤ 0.8 rules out IH (sensitivity 0.92, specificity 0.19) [2]. P2/P1 ratio ≥ 1.4 indicates IH (sensitivity 0.11, specificity 0.90) [2]. Can be reinforced with a TTP ≥ 0.3 (sensitivity 0.16, specificity 0.92) [2]. A ML model can estimate ICP values with an error of nearly 3 mmHg	Allows continuous monitoring in real time; good temporal resolution to observe responses to clinical interventions. Not restricted to use by a specific professional	Patients who are highly agitated may be unsuitable candidates for scanning	Single provider	Affordable, requires a monthly digital subscription, no disposables
TCD – PI	The device uses Doppler shift to calculate blood velocity and applies color coding to indicate flow direction and insonation angle	PI ≥ 1.4 with diastolic velocities ≤ 20 cm/s indicate IH Sensitivity = 0.74 and specificity = 0.74 regarding an optimal cut-off value of 1.28 [ESM1]	Allows multiple additional diagnostics, as brain death, arterial stenosis, emboli and the overall cerebral hemodynamic panorama	Only physicians may perform this procedure, which requires extensive training for competency. Multiple central and systemic variables influence its parameters	Several providers	One-time device purchase. No disposables

Table 1 (continued)

Technique	Principle	Cut-offs for IH/ IH indicators and sensitivity/specificity	Pros	Cons	Commercial information[a]	
TCD—nICP formula	Uses TCD blood flow velocity and ABP signal	nICP > 25 mm Hg can be considered as a threshold for intracranial hypertension Sensitivity = 0.70 and specificity = 0.70 with an optimal cut-off value of 19.6 mmHg [ESM1]	Allows continuous monitoring of ICP- mean value, respiratory, pulse and vasogenic waves	Absolute error around 9.5 mm Hg	Several providers	One-time device purchase. No disposables

CSF, cerebrospinal fluid; CT, computed tomography; CTP, CT perfusion; CTxe, Xenon CT; EEG, electroencephalogram; ICP, intracranial pressure; IH, intracranial hypertension; MRI, magnetic resonance imaging; NIRS, near-infrared spectroscopy; PI, pulsatility index; TTP, time-to-peak; ML, machine learning; TCD, transcranial Doppler; ABP, arterial blood pressure; nICP, non-invasive intracranial pressure

[a] Most hospitals have Ultrasound/TCD/EEG already, hence is less the purchase of the machine, but more the indirect cost of provider time/interpretation, etc., that might be rate-limiting, versus new purchase of a new system

These equations provide a physiologically intuitive link between systemic pressure, Doppler-derived flow distribution, and estimated ICP, being useful for trend detection and Doppler data integration into clinical decision pathways. The TCD-nICP presents a sensitivity and specificity of 0.70 for an optimal cut-off value of 19.6 mmHg [9] (ESM 1). Many studies have evaluated the validity of TCD-derived nICP. The Invasive Versus Non Invasive Measurement of Intracranial Pressure in Brain Injury Trial 2 (IMPRESSIT-2) validated the role of TCD assessments as a screening tool to exclude clinically relevant IH in ABI patients, showing high negative predictive value (NPV) compared with simultaneous invasive ICP monitoring, and reinforcing the importance of standardized acquisition and experienced operators [15]. Acoustic window failure and poor image/measurement quality may also limit applicability in a subset of patients. Mid-range ICP values remain the zone of greatest uncertainty; TCD-derived methods are most reliable for trend detection and for identifying extreme states (very low EDV or diastolic flow reversal) rather than providing precise single-point ICP numbers [16]. In order to optimize clinical use of these non-invasive techniques, TCD-nICP and PI should be integrated into a multimodal monitoring strategy including: (1) standardized TCD exams with concurrent MAP and $PaCO_2$ documentation; (2) interpretation of PI and nCPP/nICP trends alongside neurological examination and imaging; and (3) contemporary use of other devices such as pupillometry and electroencephalogram (EEG). This strategy may help reserve invasive ICP monitoring when precise numeric ICP values are required for management decisions. Another useful rule may be adopted at the bedside: if during TCD examination PI is greater than 1.5, without arterial hypotension and hypocapnia, these findings suggest that ICP is elevated. The B-ICONIC consensus proposes a set of 34 recommendations (32 of which were strong) designed to assist clinicians managing TBI patients using nICP systems plus clinical assessment, in the presence or absence of brain imaging [9]. One of the strong recommendations is the use of at least two different nICP methods integrated into the clinical exam and imaging, when available [9]. In case of severe IH, TCCD can detect changes indicative of compromised CBF progressing towards cerebral circulatory arrest (i.e., reverberating flow, systolic spikes, and disappearance of previously registered flow) and consequent brain death [17].

Transcranial Doppler: other advanced methods for nICP estimation

Transcranial Doppler ultrasonography remains a central modality for nICP estimation, with modern work converging on three physiologically and analytically distinct

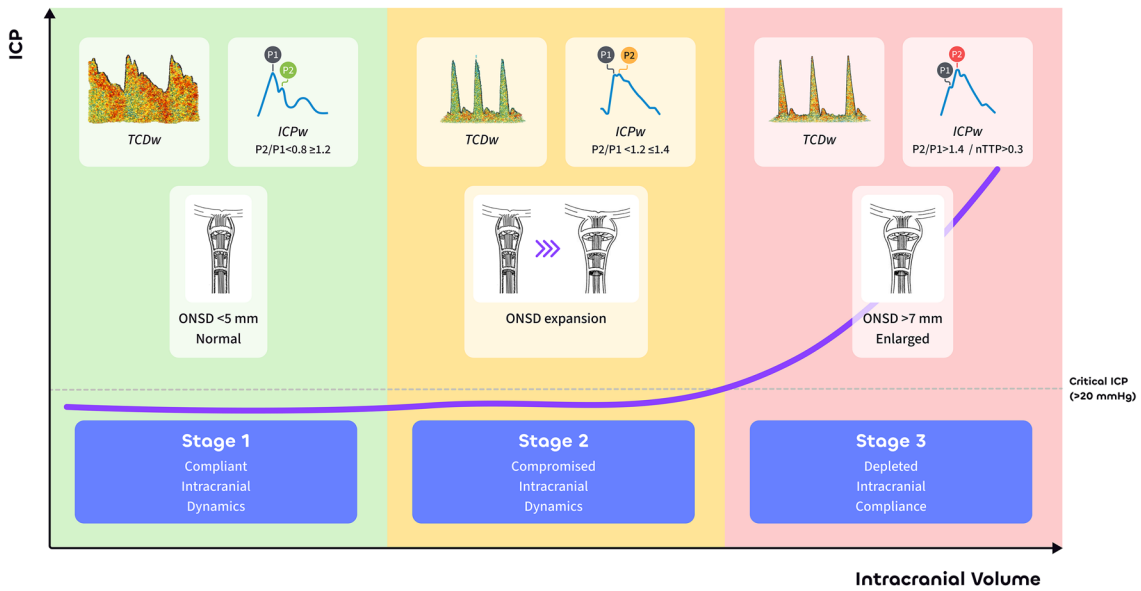

Fig. 1 Multimodal staging of intracranial compliance along the intracranial volume–pressure curve. The colored bands depict three compliance stages; the purple curve shows the exponential rise in ICP with increasing intracranial volume. The dashed horizontal line marks a commonly used clinical action level (ICP > 20 mmHg). Stage 1—compliant intracranial dynamics (green). Typical ICP waveform (ICPw) from brain4care (B4C) (with P1 ≥ P2; screening range P2/P1 ≈ 0.8–1.2. TCD waveform (TCDw) shows preserved diastolic flow without marked pulsatility. Optic nerve sheath diameter (ONSD) usually < 5 mm. Stage 2—compromised intracranial dynamics (yellow). P2 approaches or slightly exceeds P1; screening range P2/P1 ~ 1.2–1.4. ONSD shows interval expansion (~ 5–7 mm) or upward trend. TCDw often shows increased pulsatility compared with Stage 1. Stage 3—depleted intracranial compliance (pink). P2 > P1 with P2/P1 > 1.4 and nTTP > 0.30, consistent with low compliance and a higher likelihood of intracranial hypertension. ONSD > 7 mm is shown as a supportive marker. TCDw illustrates pronounced pulsatility. Abbreviations: B4C, brain4care; ICPw, intracranial pressure-related pulse morphology (P1 percussion peak; P2 tidal peak); nTTP, normalized time-to-peak; TCDw, transcranial Doppler waveform; ONSD, optic nerve sheath diameter. The direct associations between modalities are conceptual rather than definitive (i.e., despite increased ICP or reduced compliance, only some modalities may show signs of increased ICP depending on patient-specific circumstances)

strategies. Mathematical models that derive nICP from arterial blood pressure–flow relationships, including nCPP formulations, have been widely investigated [18, 19]. Although initial studies [19] suggested potential utility as screening tools, prospective validation has never been conducted. Generally, these methods cannot provide a reliable estimate of ICP values and serve only as high-NPV "rule-out" screening tools [15, 20]. Machine-learning and deep-learning methods represent the most promising evolution to date. By leveraging full arterial waveforms, arterial pressure, and electrocardiogram (ECG) timing, these models learn complex, nonlinear ICP-flow relationships unavailable to analytical formulas. Recent work (conducted, however, in a short series of patients) using domain-adversarial neural networks has achieved mean absolute errors near 3.9 mmHg, outperforming all previous TCD-based techniques and demonstrating improved detection of IH [21]. However, these tools are not universally available. A complementary venous approach using TCD focuses on deep cerebral venous outflow [22], particularly the straight sinus and basal veins. Venous TCD has shown good correlation with invasive ICP ($r = 0.54$), with further improvement when combined with optic nerve sheath diameter (ONSD) ($r = 0.81$) [23]. Despite this strong physiological signal, its clinical translation is hindered by operator dependency and technical difficulty [21, 22]. Overall, currently available approaches demonstrate the expanding utility of TCD for trend monitoring and risk stratification [15]. TCCD is also useful for the visual assessment of midline shift facilitating early diagnosis and treatment in patients with a significant intracranial mass effect [24]. Studies indicate that TCD-based nICP methods show 95% limits of agreement ranging from ± 7 mmHg to as high as ± 15 mmHg [25]. Invasive ICP probes, considering Food and Drug Administration (FDA) requirements, must instead adhere to a strict accuracy of ± 2 mmHg in the range of 0–20 mmHg. However, no TCD-based method currently matches the accuracy, reliability, or treatment-guiding capability of invasive ICP monitoring.

Optic nerve sheath diameter

Optic nerve sheath diameter ultrasonography is a nICP surrogate that takes advantage of the direct continuity of the optic nerve sheath (ONS), the CSF, and the meninges with the brain [25–28]. This network allows ICP

transmission into the ONS [25]. The ONS bulb, around 3 mm behind the globe, is the most sensitive part to ICP changes [27], which is likely due to its looser trabecular meshwork without rigid septa or pillars found in the rest of the sheath [28] (Fig. 1). However, several methodological limitations must be considered when interpreting ONSD measurements. Prolonged exposure to IH may alter the elastic properties of the optic nerve sheath, potentially affecting its ability to return to baseline dimensions. In adults, ONSD values are generally considered normal below approximately 5.2 mm and suggestive of enlargement when exceeding 5.8 mm; however, fixed cutoffs should be interpreted with caution. In the case of values between 5.2 and 5.8 mm, we suggest considering clinical picture, neuroimaging, other nICP tools, and eventually early repetition of the ONSD measurement. For ONSD-based techniques, the 95% limits of agreement range from ± 7–10 mmHg [29] which, as mentioned above, contrast with FDA requirements for invasive ICP probes. The ONSD ultrasonography presents a sensitivity and specificity of 0.83 for an optimal cut-off value of 5.9 mm [9] (ESM 1). The ONSD is also influenced by individual anthropometric characteristics, and several studies recommend normalization to eyeball diameter and/or optic nerve diameter to improve accuracy. To optimize visualization of the optic nerve trajectory, the CLOSED [Color Doppler–Low power examination–Optic disk clarity–Safety (short examination duration)–Elevate frequency–Dual measurements] protocol advocates the use of color Doppler to identify the central retinal artery and vein within the nerve [30]. In addition, many studies do not clearly specify whether the internal ONSD (ONSDint), i.e., measuring only the subarachnoid space, or the external ONSD (ONSDext), i.e., including the dural sheath, is assessed [31]. These two approaches differ substantially, with a reported mean discrepancy of approximately 22%, which limits inter-study comparability when not explicitly defined [32]. As with all ultrasound-based techniques, inter-observer variability represents an important source of measurement error. Accordingly, it is recommended to perform repeated measurements and to confirm consistency, typically defined as less than a 10% difference between values. Furthermore, ocular ultrasound should always adhere to the ALARA (As Low As Reasonably Achievable) principle to minimize acoustic exposure to the retina and lens [31]

Given these limitations, ONSD is often most informative when used for serial assessments in the same patient, comparing changes over time rather than relying on a single absolute value. Despite methodological heterogeneity, multiple meta-analyses have demonstrated that ONSD ultrasonography has good diagnostic performance for detecting intracranial hypertension, with reported sensitivities ranging from 86 to 92%, specificities from 78 to 90%, and overall diagnostic accuracy between 0.87 and 0.93 in both traumatic and non-traumatic neurocritical care populations [31, 33–35]. Recommendations to improve the utility of ONSD include: (1) following a standardized imaging and measurement checklist [36], (2) avoiding artifacts [37], (3) using machine learning to automate measurements [38], and (4) using a multimodal approach to evaluate ICP, including TCD, pupillometry, and ONSDint cut-off > 6 mm [9]. This method requires a linear probe (without adjunctive software installation), which is generally easy to find worldwide. However, this method is not always feasible after TBI because eye accessibility might not be possible.

Automated pupillometry

Automated pupillometry allows objective and comprehensive assessment of the pupillary light response (PLR) providing pupil size, percentage of pupillary constriction (%C), constriction velocity (CV), maximum contraction velocity (MCV), dilation velocity (DV), and latency response [39]. Some pupillometers also provide pupil indexes like the neurologic pupil index (NPi) and the quantitative pupillometry index (QPi), which integrate the above-mentioned parameters with a score from 0 to 5 (an NPi or a QPi < 3 is considered abnormal) (Fig. 1). Automated pupillometry presents a sensitivity and specificity of 0.68 for an optimal cut-off value of 3.96 [9] (ESM 1). Altered PLR, such as changes in pupil size and reactivity, reflects midbrain compression caused by uncal herniation, ischemia, hemorrhage, or edema [39–41]. As such, PLR parameters may be altered in case of IH with associated midbrain and/or oculomotor nerve compression. In fact, studies have reported abnormal NPi values preceding the diagnosis of uncal herniation in ABI patients [42, 43] while a significant, clinically relevant decrease in NPi often accompanies sustained episodes of IH [44, 45]. However, third cranial nerve or brainstem compression is not always present in case of elevated ICP. In fact, most cohort studies reported only a weak, clinically insignificant association between NPi reduction and ICP elevation [46–50], while a few demonstrated a moderate inverse correlation between NPi and ICP [44, 51, 52]. Moreover, Petrosino et al. demonstrated an overall lack of association between concomitant repeated NPi and invasive ICP values [50]. Therefore, as suggested by the B-ICONIC consensus, the NPi alone to assess ICP is unreliable and should only be applied in conjunction with other non-invasive methods and clinical picture to identify IH [9]. Additionally, other parameters such as CV, DV, %C, and pupil size may have a role in the nICP evaluation [41, 43, 53, 54], despite being less studied than NPi.

Non-invasive estimation of intracranial compliance

The skull may extend when ICP rises; this extension is very small but can be monitored using high-precision electronic devices. One of them is the brain4care (B4C) system, a novel non-invasive cranial extensometer designed for continuous, real-time monitoring of ICP wave (ICPW) morphology, intracranial compliance (ICC), and ICP estimation [55–60]. Technically, the B4C is a wearable device detecting beat-to-beat micrometric skull deformations from ICP variations with high sensitivity (< 0.2 µm) [61]. The proprietary algorithm extracts key ICPW parameters like the P2/P1 ratio and the time-to-peak (TTP), validated to show strong agreement with invasive measures in several single-center observational studies [55–58, 60, 62, 63]. A P2/P1 ratio of 0.8 has a 92% sensitivity to ICP rise above 20 mmHg, whereas a P2/P1 ratio of 1.4 and a TTP of 0.3 demonstrate a 90% specificity [60]. An integrated machine learning model also enabled nICP estimation with promising accuracy, which will be a possible additional information automatically provided by this system in the near future [64]. Normal values of P2/P1 ratio should be < 0.8 and TTP below 0.3 in both adult and pediatric populations. These values can increase with age and in women, with the P2/P1 ratio reaching up to 1.2 [65, 66]. Clinical studies show that a P2/P1 ratio above 1.4 is associated with a higher risk of IH [60]. These ratios relate non-linearly to ICP and may decrease after ICP reaches a critical level [63]. Initial clinical studies show broad applications of this novel methodology, which include detecting ICP elevations, assessing IH, cerebral autoregulation [67], cerebrospinal compliance [61], and brain compensatory reserve [61], providing prognostic insights to achieve better outcomes [49, 62, 68]. Its high NPV for ruling out IH makes it a valuable screening tool [60, 62]. Enhanced prognostic capabilities are observed when B4C is combined with TCD [59]. The system can capture waveforms similarly to invasive methods in patients, regardless of skull condition, including fractures, craniotomy, or craniectomy [55]. However, ICP waveform applicability when the bone flap is absent still needs further assessment [69]. The system monitors all intracranial volumes, serving as a proxy for evaluating intracranial dynamics. Changes in ICP wave patterns indicate that resistance to blood or cerebrospinal fluid flow in the brain is increased [61]. Future research on B4C should focus on extensive validation through large-scale, multicenter prospective studies across diverse patient populations to strengthen generalizability and to confirm its accuracy in various clinical scenarios. Technological advancements are crucial, including improving algorithms for ICP estimation. Clinically, future studies should investigate the system's impact on patient outcomes by guiding personalized therapies, optimizing ICP management, supporting mechanical ventilation weaning, etc.

Other methods

Neuroimaging, particularly computed tomography (CT), may show radiological signs of IH (e.g., midline shift, basal cistern effacement, and/or presence of space-occupying lesions) [70, 71]. The MRI imaging-derived elastance index (derived from the ratio of pressure to volume change) shows a promising correlation with ICP [72]. Moreover, both techniques can be utilized to estimate ONSD [73]. The presence of IH with a normal CT scan of the brain is a classic presentation of idiopathic intracranial hypertension [74]. In this regard, subtle signs of chronic high pressure are empty sella (flattening of the pituitary gland), dilatation of the optic nerve sheaths, or slit-like ventricles. Unfortunately, CT and MRI are time-consuming methods not easily useful for repeated bedside assessments.

The EEG can show changes related to IH and associated cerebral ischemia such as frequency slowing, reduced amplitude, or background disorganization [75, 76]. However, the EEG requires interpretation by trained personnel and is frequently influenced by sedative medications [75].

Intracranial pressure increments are transmitted to the optic nerve and retinal veins, inducing swelling of the optic disc and venous collapse [77]. These signs, if analyzed with a simple portable ophthalmoscope, are subjective and not always specific [77]. The optical coherence tomography (OCT) and the OCT-angiography (OCTA) can provide more objective and detailed assessments [77]. These devices are difficult to transport to the patient's bedside and require pharmacological pupil dilation (which can affect the neurological assessment for some time) [77]. A small pilot study was recently published regarding a portable instrument, but more data are needed on the applicability and reliability of this tool in daily clinical practice [78].

Intracranial components (brain, blood, and CSF) have different acoustic properties. A change of the content of these components, inside the acoustic path, influences the total acoustic characteristics of the intracranial media [79, 80]. The time-of-flight (TOF) analysis, which accounts for cranial tissue impedance, requires a specialized equipment and is not widely available in clinical practice [79, 80].

Pressure exerted from the CSF within the skull is transmitted to the perilymph within the inner ear [79, 81]. Therefore, an increase in ICP leads to a proportional increase in peri-lymphatic pressure, which can be measured non-invasively by the tympanic membrane

displacement [79, 81, 82]. More studies are necessary to validate this technique in daily clinical practice.

Another nICP measurement method is based on a two-depth high-resolution transcranial Doppler insonation of the ophthalmic artery. The artery is used as a natural pair of scales, in which the intracranial segment of the artery is compressed by ICP and the extracranial segment is compressed by extracranial pressure (Pe) applied to the orbit. The blood flow parameters in both ophthalmic artery segments are approximately the same when Pe = ICP. A specialized monitor has been constructed and tested clinically [83].

Clinical applications

Neuro-intensive care (when ICP is available)

In patients with severe TBI or SAH, nICP assessment may primarily help to refine patient selection for invasive monitoring (Fig. 2). Only about one-third of TBI patients who meet guideline-based monitoring criteria ultimately develop sustained IH [84]. Similarly, in SAH, EVDs are often placed for altered consciousness or hydrocephalus, although significant brain edema may also occur in the absence of CSF accumulation [85]. In ischemic or hemorrhagic stroke, decisions regarding ICP monitoring are usually based on hematoma or infarct size, yet international practices remain highly variable and potential survival implications have been reported [86, 87]. Earlier identification of candidates for direct ICP monitoring based on nICP assessment may facilitate timely recognition of midline shift before herniation and potentially support optimal decisions regarding brain imaging, neurosurgical intervention or escalation of medical therapy. Non-invasive monitoring may help identify such complications and/or discuss the personalized implementation of invasive monitoring. Furthermore, nICP assessment may support timely decision-making in moderate TBI or other at-risk patients who do not fulfill formal criteria for invasive monitoring, enabling earlier identification of candidates for ICP monitoring with higher accuracy. In cases of unclear decreased consciousness, nICP may help determine whether an emergency CT is necessary or whether alternative diagnoses (e.g., delirium) or diagnostics (e.g., EEG) should be prioritized first. Also, nICP is particularly valuable when invasive monitoring is contraindicated or unsafe, such as in the presence of coagulopathy (e.g., polytrauma), anticoagulation (e.g., hemorrhagic stroke), or dual antiplatelet therapy (e.g., SAH treated with intracranial stents), as it would allow safe interim surveillance until definitive monitoring becomes feasible. Finally, in patients already undergoing invasive monitoring, concurrent nICP assessment may contribute to individualized treatment thresholds and strategies (e.g., quantifying the tolerability of the brain to a specific ICP value rather than protocol-driven care based on fixed thresholds, hyperemia contributing to IH, etc.) (Fig. 3).

There is currently no evidence that pre-screening patients with non-invasive methods prior to invasive ICP probe placement is cost-effective or improves outcomes. In the Benchmark Evidence from South American Trials: Treatment of Intracranial Pressure (BEST-TRIP) trial [84], the group managed with imaging- and clinical-based strategies underwent more brain-specific diagnostics and interventions, without significant difference in 6-month survival or neurological outcome. In some situations, rapid placement of an invasive probe might simply be more convenient.

In some cases, the implementation of non-invasive tools was found to be associated with unintended adverse effects. For example, Hollingworth et al. [88] reported worse long-term outcomes in centers that used routine TCD screening in addition to the standard of care, compared to those that did not, in a cohort of over 2.000 aSAH patients.

General ICU population: cardiac arrest, liver failure, mechanical ventilation, sepsis

In the general ICU population, brain injury may arise from distinct mechanisms and is increasingly recognized as a key determinant of outcome (ESM 1) [89–92]. Following cardiac arrest, global ischemia–reperfusion induces a primary insult that is subsequently aggravated by secondary brain injury caused by IH [93], easily overlooked in the absence of proper nICP methodology. In conditions such as acute respiratory failure (ARF), liver failure, sepsis, or during mechanical ventilation, secondary brain injury can develop due to systemic derangements or elevated intrathoracic pressures, even in the absence of ABI at admission [94–101]. In this context, non-invasive neuromonitoring tools, such as ONSD ultrasonography, TCD/transcranial color-coded duplex (TCCD), and automated pupillometry, provide complementary information on ICP, cerebral perfusion, autoregulation, and brainstem function. These techniques complement each other by capturing different aspects of cerebral physiology: vascular resistance, edema, and brainstem reflexes. Following cardiac arrest, ischemia–reperfusion injury triggers cytotoxic and vasogenic edema, impaired autoregulation, and, in some cases, IH [93]. The CBF decreases immediately after the return of spontaneous circulation (ROSC) but generally normalizes within 72 h, with more pronounced reductions in severe hypoxic–ischemic encephalopathy (HIE) [102, 103]. Transcranial Doppler-derived indices, including PI and estimated CPP, reflect intracranial compliance and perfusion after ROSC. In a recent study, a PI ≥ 1.49 was

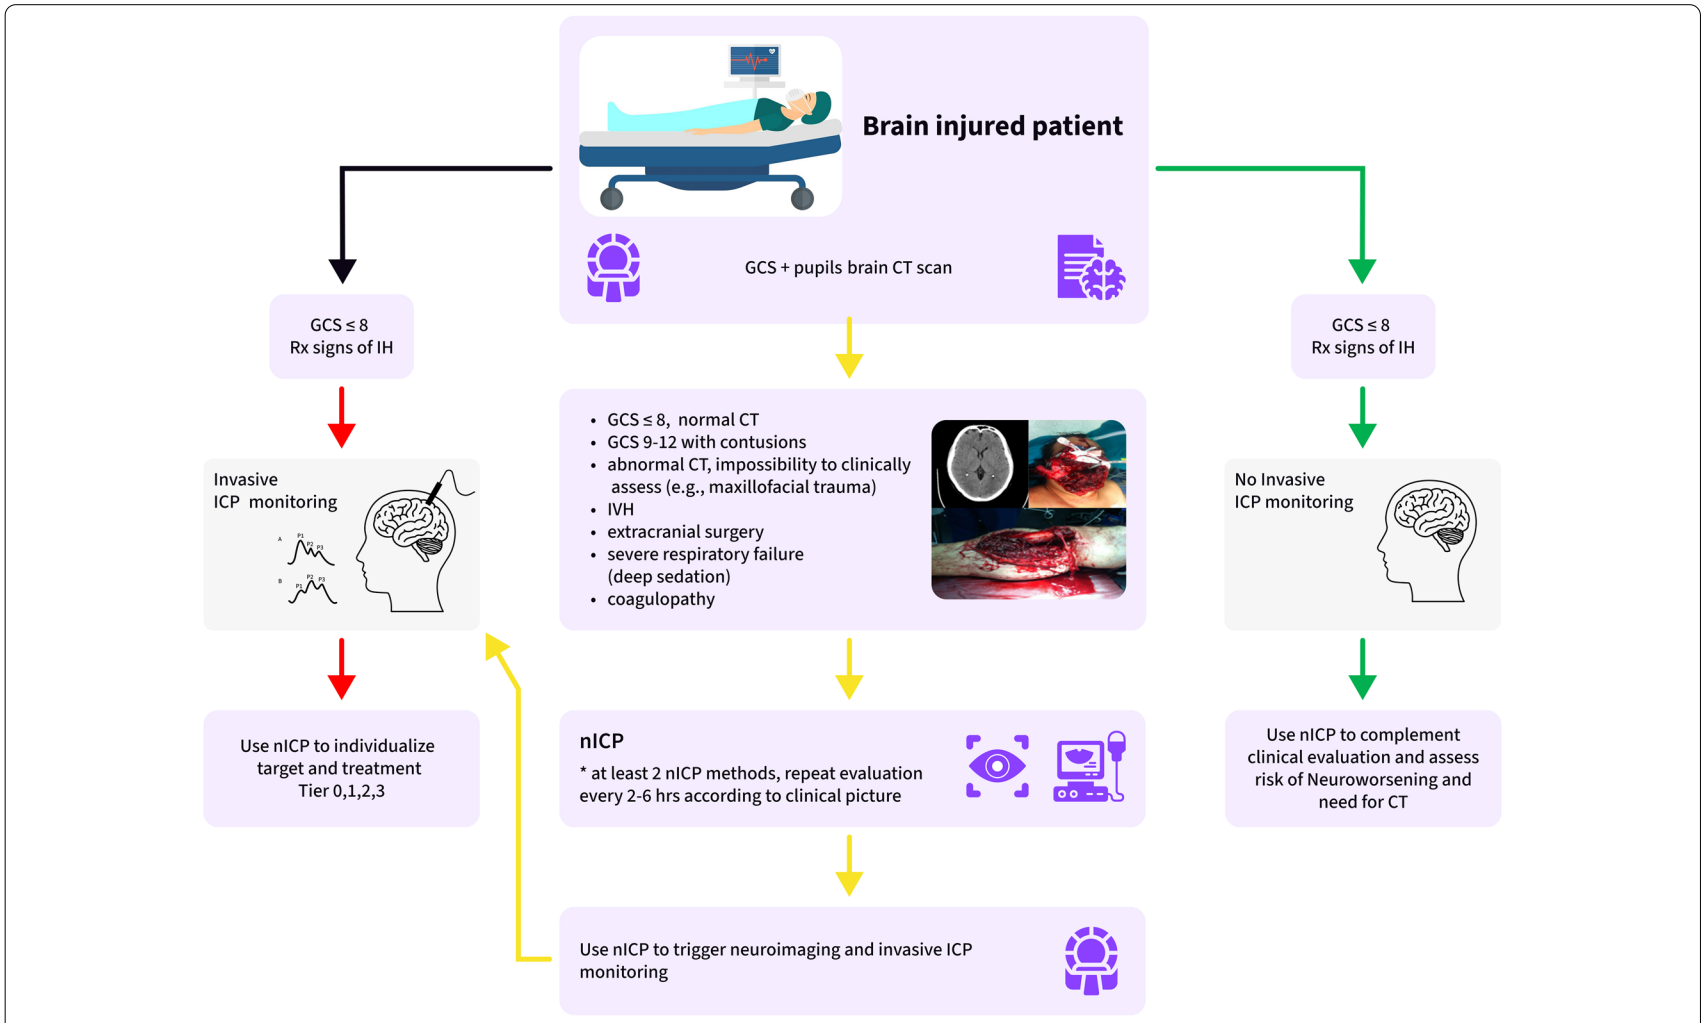
Brain injured patient
GCS + pupils brain CT scan
GCS ≤ 8
Rx signs of IH
GCS ≤ 8
Rx signs of IH
• GCS ≤ 8, normal CT
• GCS 9-12 with contusions
• abnormal CT, impossibility to clinically assess (e.g., maxillofacial trauma)
• IVH
• extracranial surgery
• severe respiratory failure (deep sedation)
• coagulopathy
Invasive
ICP monitoring
No Invasive
ICP monitoring
Use nICP to individualize target and treatment Tier 0,1,2,3
nICP
* at least 2 nICP methods, repeat evaluation every 2-6 hrs according to clinical picture
Use nICP to complement clinical evaluation and assess risk of Neuroworsening and need for CT
Use nICP to trigger neuroimaging and invasive ICP monitoring

Fig. 2 Potential use for the application of non-invasive intracranial pressure monitoring (nICP) tools in patients with acute brain injury when ICP is available. After initial assessment (Glasgow Coma Scale, GCS, and neuroimaging), in patients with severe brain injury (i.e., GCS < 9), nICP could help to better select patients for invasive intracranial pressure (ICP) monitoring, or to monitor those with contraindications to invasive ICP, or to individualize ICP thresholds for therapeutic interventions. In mild-to-moderate injury, nICP might help to identify patients with the highest risk of intracranial hypertension, risk of neuro-worsening and need for imaging and invasive tools. Abbreviations: TBI = traumatic brain injury, IH = intracranial hypertension, nICP = non-invasive intracranial pressure; GCS, Glasgow Coma Scale; CT, Computed Tomography; IVH, intraventricular haemorrhage

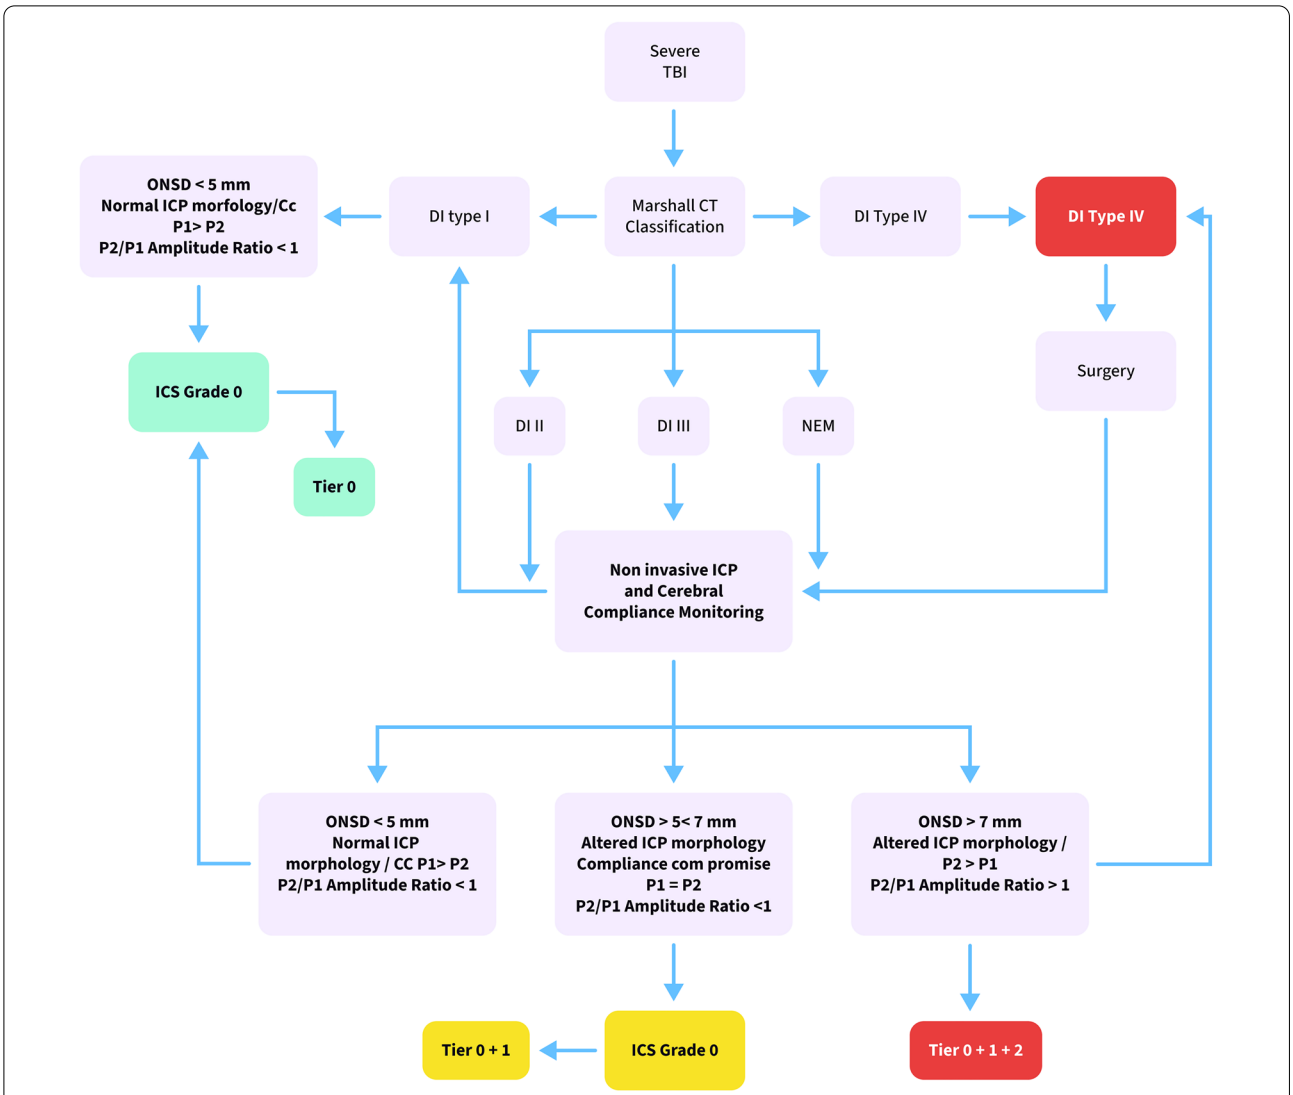

Fig. 3 PARADIGM Protocol (supported by intracranial compartment syndrome and developed with computed imaging scan findings (Marshall's classification*) and non-invasive neuromonitoring, for the management of acute brain injured patients when invasive ICP is not available. TBI: traumatic brain injury; DI: diffuse injury; ICP: intracranial pressure; CC: cerebral compliance; ICS: intracranial compartment syndrome; NEML: non-evacuated mass lesion; ONSD: optic nerve sheath diameter. *Marshall LF, Marshall SB, Klauber MR, van Berkum Clark M. A new classification of head injury based on computerized tomography. J Neurosurg. 1991; 75(Suppl): S14–20

significantly associated with poor neurological outcome [104]. In another prospective study, TCD-based ICP estimation showed a significant, albeit moderate, correlation with invasive ICP and a high predictive value for IH [97]. In the same study, ONSD demonstrated the strongest correlation with invasively measured ICP and an excellent accuracy in detecting IH [105]. The PLR assessed through quantitative pupillometry is a reliable prognostic marker after ROSC. A NPi ≤ 2 within 6 h after cardiac arrest strongly predicts poor neurological outcome [106, 107], with persistence at 72 h being highly specific [108, 109]. Thus, quantitative pupillometry complements EEG and somatosensory-evoked potentials in neuro-prognostication [110].

Cerebral edema and IH are devastating complications of acute liver failure, with an incidence of approximately 30% [111, 112]. Invasive ICP is contraindicated in the case of coagulopathy, making non-invasive approaches the safest alternative in this setting. In adults, ONSD and PI have shown limited diagnostic accuracy, whereas TCD-derived nICP demonstrated excellent performance with a high NPV [113]. In children, ONSD has been shown to predict mortality [114], and prospective data indicate that an ONSD > 4.55 mm

reliably identifies raised ICP, while failure to reduce it below 4.6 mm within 24 h predicts poor outcomes [115]. These modalities may also guide timely escalation of interventions, including osmotherapy or ammonia-lowering treatments.

The complex interplay between the brain and lungs has critical implications in ARF patients. Hypercapnia and hypoxemia directly influence CBF, with TCD/TCCD-derived FVm and PI providing reliable bedside correlations with oxygen content and $ETCO_2$ [116–120]. The impact of positive end-expiratory pressure (PEEP) on ICP and CPP is influenced by the lung recruitability and the cerebral autoregulation status. When PEEP induces alveolar overdistension, the subsequent rise in intrathoracic pressure may increase ICP and reduce CPP. Conversely, when PEEP promotes effective alveolar recruitment, oxygenation can improve without increasing intrathoracic pressure, thereby minimizing harmful cerebral effects [97–99, 121–124]. The TCD/TCCD assessment enables clinicians to identify deleterious responses—such as elevated PI or nICP and reduced CBF—and to guide individualized PEEP titration [121]. The application of prone positioning (PP) may add further challenges: in the acute respiratory distress syndrome (ARDS), even in the absence of ABI, standard PP has been associated with increased PI, which can be mitigated by a 30° reverse-Trendelenburg 'head-up' PP [125]. Similarly, in ARDS patients with ABI, tailoring head inclination during PP guided by TCD monitoring may help to mitigate ICP increase [126, 127]. Some non-invasive tools (e.g., TCCD, pupillometry, etc.) could be useful for neuromonitoring in patients undergoing extracorporeal membrane oxygenation support [128].

The TCD-derived nCPP (i.e., estimated CPP) was found to be reduced in one-third of a cohort of 132 septic patients; however, these alterations were not associated with the development of sepsis-associated encephalopathy (SAE) or with in-hospital mortality [129]. In contrast, an ONSD > 5.2 mm has shown high predictive value for SAE [130]. Moreover, TCD is essential for assessing cerebral autoregulation which is an independent predictor of SAE [131].

Generally, it is important to underline how none of the described methods has been validated specifically in these populations; most development and validation studies focus on TBI cohorts. Further studies should be performed in these settings.

Pre-hospital and emergency department settings (potential applications before to arrive in the ICU)

The very early phase following an acute cerebral insult can critically influence patient outcomes, particularly in the presence of IH, which, if unrecognized, may rapidly progress to fatal neurological deterioration. In the prehospital setting, where invasive ICP monitoring is not available, non-invasive assessment techniques could potentially play a fundamental role in the early identification of IH. Initial patient evaluation primarily focuses on detecting clinical features suggestive of raised ICP, including headache, nausea, vomiting, and visual disturbances. Suspicion should be further heightened in the presence of reduced level of consciousness, abnormal pupillary light reflexes, systemic arterial hypertension with widened pulse pressure, tachycardia followed by bradycardia, and irregular respiratory patterns [132, 133]. However, it is important to recognize that classical signs such as pupillary abnormalities, arterial hypertension, and bradycardia have limited sensitivity for identifying IH in the prehospital environment, particularly in the early stages [134, 135].

For the rapid assessment of comatose patients, automated pupillometry could represent a valuable first-line tool. It allows objective, quantitative evaluation of bilateral pupillary light reflexes within a few seconds, providing insight into midbrain function, and can be repeated frequently without operator dependency. In the subsequent minutes, either at the scene, during ambulance transport or in the emergency department, additional complementary non-invasive assessments can be performed. Available non-invasive cranial extensometers offer practical advantages in these settings, as they do not require a physician or specialized operator and allow hands-free application. Once installed, reliable signal acquisition can be achieved within approximately one minute. Importantly, this technology enables continuous or intermittent monitoring over prolonged periods, assessing intracranial compliance through waveform analysis. This could allow early detection of IH, monitoring of its progression, evaluation of responses to therapeutic interventions, and longitudinal comparisons over time. Ultrasound-based techniques, although examiner-dependent, could also be implemented early; ONSD measurement and TCD/TCCD could provide valuable information. Unilateral ONSD enlargement may suggest ICP gradients, whereas bilateral enlargement is more consistent with acute and severe IH [136, 137]. TCD/TCCD enable indirect estimation of ICP through parameters such as PI and FVd, while insonation of the MCAs offers a rapid overview of global cerebral hemodynamics and remains particularly useful in the evaluation of acute stroke [136, 137]. Although more studies are needed in these settings to draw reliable recommendations, the use of nICP tools, in experienced hands and integrated with clinical and radiological examination [138–140], could facilitate timely recognition of IH allowing early intervention. Early IH detection, even before imaging, could

allow clinicians to mitigate the risk of cerebral herniation during patient transport or positioning and to prevent secondary brain injury related to inadequate sedation, uncontrolled arterial pressure, or inappropriate $PaCO_2$ levels. Future research should also focus on the broader integration of portable, non-invasive monitoring technologies into prehospital and emergency care pathways. At present, insufficient data are available regarding the utilization of nICP methods in the prehospital setting making future study on this topic auspicable. However, the use of non-invasive tools must not slow down the execution of brain CT scans which play a key role in the assessment of these patients in the acute phase. Non-invasive tools can potentially be useful in polytrauma TBI patients needing emergent extracranial surgery for bleeding control. In these difficult situations their application should not interfere with life-saving interventions and would require extremely trained and coordinated personnel. This topic should definitely be the subject of further studies in the future.

Low-income countries: when invasive ICP monitoring is not available

Traumatic brain injury remains a major health concern worldwide, with therapeutic strategies and prognosis varying according to resource availability [141]. In limited resource settings, neuro-intensive care faces major challenges, particularly where advanced neuromonitoring tools, such as invasive ICP, are unavailable [142, 143]. In this scenario, clinicians traditionally rely primarily on neurological examination and neuroimaging, as shown by different protocols [i.e., the Imaging and Clinical Examination (ICE) protocol, the Consensus REVised ICE (CREVICE) protocol, and the Beyond One Option for Treatment of Traumatic Brain Injury: A Stratified Protocol (BOOTStraP)] [84, 144–147]. In particular, the ICE and the CREVICE protocols have been validated in clinical practice and are associated with improved neurological outcomes [145, 146]. However, clinical assessments are often late indicators of IH (e.g., posturing, arterial blood pressure fluctuations, etc.), limiting timely and targeted interventions. Brain CT scan, when available, assists in detecting mass effect, midline shift, basal cisterns status, or hydrocephalus, but its use is constrained by high costs, limited availability, and the risks associated with the transport of critically ill patients [140, 148]. Consequently, non-invasive neuromonitoring has emerged as a practical, affordable, and useful alternative [143, 149]. However, in this regard, we await new studies regarding nICP in low-resource settings and the validation in clinical practice of the recently published B-ICONIC consensus [9]. As recommended, some methods may be more useful when applied repeatedly within the same patient. This may partly explain why their use often remains limited to experienced users in specialized settings rather than translating into broader benefit for less specialized and less resource-intensive centers. Moreover, individually, several methods have yielded negative results, underscoring the nuanced background knowledge required for appropriate use and interpretation. Until invasive ICP monitoring becomes universally accessible, non-invasive neuromonitoring optimization and basic neurocritical care knowledge appear to be useful tools for improving neurological outcomes in poor resource settings.

Most currently available nICP monitoring approaches do not provide truly continuous precise measurements. Instead, they primarily aim to predict whether a predefined (invasive) ICP threshold is exceeded. However, over the past decade, research has repeatedly demonstrated that fixed ICP thresholds are unlikely to be universally valid [150]. Increasing evidence suggests that outcome prediction is better captured by the cumulative "ICP dose", reflecting both the magnitude and duration of ICP elevation. To date, none of the proposed nICP monitoring strategies appears to address this paradigm shift or to account for the temporal dimension of ICP burden.

Large studies capturing the effect of specific interventions (e.g., hyperosmolar therapy) on nICP parameters are lacking. This is an area of research that should be implemented in the future.

Other (austere environment)

Guidelines have traditionally been created to manage ABI patients in optimally resourced environments. Organizations, like the Brain Trauma Foundation (BTF), now recognize that resource stratification efforts must be a part of guidelines going forward to better serve patients worldwide [151]. In modern combat casualty care, we face not only the challenge of providing the best possible care to patients with brain injuries, despite limited resources, but also that of providing it under fire [151, 152]. In this case, weight and volume are key factors, as a limiting factor is the carrying capacity of military medics' backpacks. Recent years have seen important advancement in technologies that hold promise for bridging the gap of optimizing care when invasive ICP measurements are not feasible [151]. Point-of-care testing for blood-based biomarkers and hand-held portable spectroscopy devices may assist the diagnosis of TBI and, in particular, the detection of intracranial blood when CT scanning is not available [153–155]. Non-invasive ICP tools could be useful in this scenario. In particular, the automated pupillometry has been introduced as a possible monitoring tool in the recently published "Joint Trauma System Clinical Practice Guideline" on the "Traumatic Brain Injury

Management and Basic Neurosurgery in the Deployed Environment" [152]. Specifically, a NPi < 3 in one or both eyes may be related to IH [152]. More efforts are needed in this area, especially to improve the monitoring and subsequent treatment of TBI patients in austere environments. Especially in battlefield, rapid evacuation ("load and go") may be lifesaving, compared to prolonged on-site assessment with nICP devices. This aspect warrants further studies.

Conclusions

Over the past decades, substantial progress has been made in the recognition and prediction of raised ICP without the need for direct monitoring. These advances have converged into the development of nICP estimation techniques, which have gained increasing interest as safe, inexpensive, bedside, and readily available tools to support the management of patients with or at risk of IH. Although their intrinsic limitations, mainly limited accuracy, prevent them from being reliable substitutes for invasive systems, these techniques can be effectively employed when invasive methods are unavailable or contraindicated, and as complementary tools to improve the understanding of intracerebral dynamics. Further research is needed to provide evidence on the impact of therapeutic strategies guided by non-invasive monitoring, particularly when integrated with neurological examination and radiological assessment.

Supplementary Information
The online version contains supplementary material available at https://doi.org/10.1007/s00134-026-08420-7.

Author details
[1] Department of Anesthesia and Intensive Care, Parma University Hospital, Parma, Italy. [2] Department of Clinical Science and Translational Medicine, "Tor Vergata" University of Rome, Rome, Italy. [3] Department of Intensive Care, Erasme Hospital, Université Libre de Bruxelles, Brussels, Belgium. [4] Division of Neurosurgery, Department of Neurology, School of Medicine, University of São Paulo, São Paulo, Brazil. [5] Department of Neurology, University of Texas Southwestern Medical Center, Dallas, USA. [6] Institute for Exercise and Environmental Medicine, Texas Health Presbyterian Hospital, Dallas, USA. [7] Department of Clinical Neurosciences, University of Cambridge, Cambridge, UK. [8] Neuroscience Institute, Universidad El Bosque, Bogota, Colombia. [9] Cleveland Clinic Lerner College of Medicine of Case Western Reserve University School of Medicine, Cleveland, USA. [10] Department of Neurology and Neurosurgery, Baylor College of Medicine, Houston, USA. [11] Center for Space Medicine, Baylor College of Medicine, Houston, USA. [12] Department of Medical and Surgical Specialties, Radiological Sciences and Public Health, University of Brescia, Brescia, Italy. [13] Department of Neuroanesthesia, Neurocritical and Post-Operative Care, ASST Spedali Civili University Hospital, Brescia, Italy. [14] Department of Emergency and Trauma, Faculdade de Medicina, Universidade Federal de Ciências da Saúde de Porto Alegre, Porto Alegre, Brazil. [15] Intensive Care Unit, Hospital Cristo Redentor, Porto Alegre, Brazil. [16] IRCCS, Policlínico San Martino, Genoa, Italy.

Funding
Open access funding provided by Università degli Studi di Genova within the CRUI-CARE Agreement.

Data availability
Not applicable.

Declarations

Conflict of interest
Carla Rynowski: Senior advisor for Brain 4Care. Chiara Robba is a Deputy Editor for Intensive Care Medicine. She has not taken part in the review or selection process of this article.

Open Access
This article is licensed under a Creative Commons Attribution-NonCommercial 4.0 International License, which permits any non-commercial use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit http://creativecommons.org/licenses/by-nc/4.0/.

Publisher's Note

Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.

Received: 17 January 2026 Accepted: 30 March 2026
Published online: 27 April 2026

References

1. Hawryluk GWJ, Citerio G, Hutchinson P et al (2022) Intracranial pressure: current perspectives on physiology and monitoring. Intensive Care Med 48(10):1471–1481
2. The Brain Trauma Foundation. The American Association of Neurological Surgeons. The Joint Section on Neurotrauma and Critical Care (2000) Indications for intracranial pressure monitoring. J Neurotrauma 17(6–7): 479–91.
3. Brain Trauma Foundation; American Association of Neurological Surgeons; Congress of Neurological Surgeons (2007) Guidelines for the management of severe traumatic brain injury. J Neurotrauma 24 Suppl 1: S1–106.
4. Carney N, Totten AM, O'Reilly C et al (2017) Guidelines for the Management of Severe Traumatic Brain Injury. Fourth Edition Neurosurgery 80(1):6–15
5. Picetti E, Galarza L, Arroyo Diez M, et al; Triple T study group (2025) Staircase strategy, tier-three therapies, and effects on outcome in traumatic brain injured patients: the Triple-T TBI study. Intensive Care Med 51(4): 681–691.
6. Robba C, McCredie V, Chesnut RM et al (2025) Traumatic brain injury management in the intensive care unit: standard of care and knowledge gaps. Intensive Care Med 51(6):1112–1127
7. Robba C, Frigieri G, Brasil S, Taccone FS (2022) Early prognostic value of non-invasive intracranial pressure methods in brain-injured patients. Intensive Care Med 48(12):1812–1814
8. Brasil S, Chesnut R, Robba C (2024) Noninvasive neuromonitoring in acute brain injured patients. Intensive Care Med 50(6):960–963
9. Robba C, Picetti E, Vásquez-García S et al (2025) The Brussels consensus for non-invasive ICP monitoring when invasive systems are not available in the care of TBI patients (the B-ICONIC consensus, recommendations, and management algorithm). Intensive Care Med 51(1):4–20
10. Bellner J, Romner B, Reinstrup P, Kristiansson KA, Ryding E, Brandt L (2004) Transcranial Doppler sonography pulsatility index (PI) reflects intracranial pressure (ICP). Surg Neurol 62(1):45–51

11. de Riva N, Budohoski KP, Smielewski P et al (2012) Transcranial Doppler pulsatility index: what it is and what it isn't. Neurocrit Care 17(1):58–66
12. ICM+ (Cambridge Enterprise). Non-Invasive Intracranial Pressure Monitoring (TCD-based nICP) overview and methodology description, ICM+ resource pages. https://icmplus.neurosurg.cam.ac.uk.
13. Czosnyka M, Matta BF, Smielewski P, Kirkpatrick PJ, Pickard JD (1998) Cerebral perfusion pressure in head-injured patients: a noninvasive assessment using transcranial Doppler ultrasonography. J Neurosurg 88(5):802–808
14. Schmidt EA, Czosnyka M, Matta BF, Gooskens I, Piechnik S, Pickard JD (2000) Non-invasive cerebral perfusion pressure (nCPP): evaluation of the monitoring methodology in head injured patients. Acta Neurochir Suppl 76:451–452
15. Rasulo FA, Calza S, Robba C et al (2022) Transcranial Doppler as a screening test to exclude intracranial hypertension in brain-injured patients: the IMPRESSIT-2 prospective multicenter international study. Crit Care 26(1):110
16. Robba C, Cardim D, Sekhon M et al (2018) Transcranial Doppler: a stethoscope for the brain-neurocritical care use. J Neurosci Res 96(4):720–730
17. Deana C, Biasucci DG, Aspide R et al (2024) Transcranial Doppler and Color-Coded Doppler Use for Brain Death Determination in Adult Patients: A Pictorial Essay. J Ultrasound Med 43(5):979–992
18. Cardim D, Robba C, Bohdanowicz M et al (2016) Non-invasive Monitoring of Intracranial Pressure Using Transcranial Doppler Ultrasonography: Is It Possible? Neurocrit Care 25(3):473–491
19. Rajajee V (2024) Noninvasive Intracranial Pressure Monitoring: Are We There Yet? Neurocrit Care 41(2):332–338
20. Rasulo FA, Bertuetti R, Robba C et al (2017) The accuracy of transcranial Doppler in excluding intracranial hypertension following acute brain injury: a multicenter prospective pilot study. Crit Care 21(1):44
21. Megjhani M, Terilli K, Weinerman B et al (2023) A Deep Learning Framework for Deriving Noninvasive Intracranial Pressure Waveforms from Transcranial Doppler. Ann Neurol 94(1):196–202
22. Schoser BG, Riemenschneider N, Hansen HC (1999) The impact of raised intracranial pressure on cerebral venous hemodynamics: a prospective venous transcranial Doppler ultrasonography study. J Neurosurg 91(5):744–749
23. Robba C, Cardim D, Tajsic T et al (2017) Ultrasound non-invasive measurement of intracranial pressure in neurointensive care: A prospective observational study. PLoS Med 14(7):e1002356
24. Motuel J, Biette I, Srairi M, et al (2014) Assessment of brain midline shift using sonography in neurosurgical ICU patients. Crit Care Dec 9; 18(6):676.
25. Martínez-Palacios K, Vásquez-García S, Fariyike OA, Robba C, Rubiano AM (2024) Non-Invasive Methods for Intracranial Pressure Monitoring in Traumatic Brain Injury Using Transcranial Doppler: A Scoping Review. J Neurotrauma 41(11–12):1282–1298
26. Aggarwal S, Knight DK, Boisvert CJ (2018) Measuring Optic Nerve Sheath Diameter as a Proxy for Intracranial Pressure. JAMA Ophthalmol 136(11):1310
27. Hansen HC, Helmke K (1996) The subarachnoid space surrounding the optic nerves. An ultrasound study of the optic nerve sheath. Surg Radiol Anat 18(4): 323–8.
28. Killer HE, Laeng HR, Flammer J, Groscurth P (2003) Architecture of arachnoid trabeculae, pillars, and septa in the subarachnoid space of the human optic nerve: anatomy and clinical considerations. Br J Ophthalmol 87(6):777–781
29. Martínez-Palacios K, Vásquez-García S, Fariyike OA, Robba C, Rubiano AM; noninvasive ICP monitoring international consensus group (2024) Using Optic Nerve Sheath Diameter for Intracranial Pressure (ICP) Monitoring in Traumatic Brain Injury: A Scoping Review. Neurocrit Care 40(3): 1193–1212.
30. Aspide R, Bertolini G, Albini Riccioli L, Mazzatenta D, Palandri G, Biasucci DG (2020) A Proposal for a New Protocol for Sonographic Assessment of the Optic Nerve Sheath Diameter: The CLOSED Protocol. Neurocrit Care 32(1):327–332
31. Dubourg J, Javouhey E, Geeraerts T, Messerer M, Kassai B (2011) Ultrasonography of optic nerve sheath diameter for detection of raised intracranial pressure: a systematic review and meta-analysis. Intensive Care Med 37(7):1059–1068
32. Lochner P, Behnke S, Fassbender K et al (2019) Simulation and Experimental Characterization of Lateral Imaging Resolution of Ultrasound Systems and Assessment of System Suitability for Acoustic Optic Nerve Sheath Diameter Measurement. J Neuroimaging 29(1):34–41
33. Ohle R, McIsaac SM, Woo MY, Perry JJ (2015) Sonography of the Optic Nerve Sheath Diameter for Detection of Raised Intracranial Pressure Compared to Computed Tomography: A Systematic Review and Meta-analysis. J Ultrasound Med 34(7):1285–1294
34. Kim EJ, Koo BN, Choi SH, Park K, Kim MS (2018) Ultrasonographic optic nerve sheath diameter for predicting elevated intracranial pressure during laparoscopic surgery: a systematic review and meta-analysis. Surg Endosc 32(1):175–182
35. Bhargava V, Tawfik D, Tan YJ, Dunbar T, Haileselassie B, Su E (2020) Ultrasonographic Optic Nerve Sheath Diameter Measurement to Detect Intracranial Hypertension in Children With Neurological Injury: A Systematic Review. Pediatr Crit Care Med 21(9):e858–e868
36. Hirzallah MI, Lochner P, Hafeez MU et al (2024) Optic Nerve Sheath Diameter Point-of-Care Ultrasonography Quality Criteria Checklist: An International Consensus Statement on Optic Nerve Sheath Diameter Imaging and Measurement. Crit Care Med 52(10):1543–1556
37. Hirzallah MI, Sarwal A, Dentinger AM et al (2025) Ultrasonographic Optic Nerve Sheath Diameter Technical Pitfalls and Imaging Artifacts. J Ultrasound Med 44(6):1103–1120
38. Escamilla-Ocañas CE, Morales-Cardona NC, Sagreiya H, Akhbardeh A, Hirzallah MI (2025) Automation of Ultrasonographic Optic Nerve Sheath Diameter Measurement: A Scoping Review. J Neuroimaging 35(1):e70017
39. Mathur R, Meyfroidt G, Robba C, Stevens RD (2024) Neuromonitoring in the ICU what, how and why? Curr Opin Crit Care 30(2):99–105
40. Manley GT, Larson MD (2002) Infrared pupillometry during uncal herniation. J Neurosurg Anesthesiol 14(3):223–228
41. Taylor WR, Chen JW, Meltzer H et al (2003) Quantitative pupillometry, a new technology: normative data and preliminary observations in patients with acute head injury. Technical note J Neurosurg 98(1):205–213
42. Papangelou A, Zink EK, Chang WW et al (2018) Automated Pupillometry and Detection of Clinical Transtentorial Brain Herniation: A Case Series. Mil Med 183(1–2):e113–e121
43. Lee H, Choi SH, Park B, Hong YH, Lee HB, Jeon SB (2021) Quantitative assessments of pupillary light reflexes in hospital-onset unresponsiveness. BMC Neurol 21(1):234
44. Jahns FP, Miroz JP, Messerer M et al (2019) Quantitative pupillometry for the monitoring of intracranial hypertension in patients with severe traumatic brain injury. Crit Care 23(1):155
45. Pansell J, Hack R, Rudberg P, Bell M, Cooray C (2022) Can Quantitative Pupillometry be used to Screen for Elevated Intracranial Pressure? A Retrospective Cohort Study Neurocrit Care 37(2):531–537
46. Stevens AR, Su Z, Toman E, Belli A, Davies D (2019) Optical pupillometry in traumatic brain injury: neurological pupil index and its relationship with intracranial pressure through significant event analysis. Brain Inj 33(8):1032–1038
47. Singer KE, Wallen TE, Jalbert T et al (2021) Efficacy of Noninvasive Technologies in Triaging Traumatic Brain Injury and Correlating With Intracranial Pressure: A Prospective Study. J Surg Res 262:27–37
48. McNett M, Moran C, Grimm D, Gianakis A (2018) Pupillometry Trends in the Setting of Increased Intracranial Pressure. J Neurosci Nurs 50(6):357–361
49. Al-Obaidi SZ, Atem FD, Stutzman SE, Olson DM (2019) Impact of Increased Intracranial Pressure on Pupillometry: A Replication Study. Crit Care Explor 1(10):e0054
50. Petrosino M, Gouvêa Bogossian E, Rebora P et al (2025) Neurological Pupil Index and Intracranial Hypertension in Patients With Acute Brain Injury: A Secondary Analysis of the ORANGE Study. JAMA Neurol 82(2):176–184
51. Robba C, Pozzebon S, Moro B, Vincent JL, Creteur J, Taccone FS (2020) Multimodal non-invasive assessment of intracranial hypertension: an observational study. Crit Care 24(1):379
52. Natzeder S, Mack DJ, Maissen G, Strässle C, Keller E, Muroi C (2019) Portable Infrared Pupillometer in Patients With Subarachnoid Hemorrhage: Prognostic Value and Circadian Rhythm of the Neurological Pupil Index (NPi). J Neurosurg Anesthesiol 31(4):428–433

53. Ali AMS, Gul W, Sen J, Hewitt SJ, Olubajo F, McMahon C (2024) Evaluating the utility of quantitative pupillometry in a neuro-critical care setting for the monitoring of intracranial pressure: A prospective cohort study. Clin Neurol Neurosurg 239:108215
54. Sandroni C, Citerio G, Taccone FS (2022) Automated pupillometry in intensive care. Intensive Care Med 48(10):1467–1470
55. Brasil S, Solla DJF, Nogueira RC, Teixeira MJ, Malbouisson LMS, Paiva WDS (2021) A Novel Noninvasive Technique for Intracranial Pressure Waveform Monitoring in Critical Care. J Pers Med 11(12):1302
56. de Moraes FM, Rocha E, Barros FCD et al (2022) Waveform Morphology as a Surrogate for ICP Monitoring: A Comparison Between an Invasive and a Noninvasive Method. Neurocrit Care 37(1):219–227
57. Uysal SP, Williams HG, Huerta M, Thompson NR, Hassett CE (2025) Noninvasive Method Using Mechanical Extensometer for the Estimation of Intracranial Compliance by Repeated Measures Agreement Analysis. Neurocrit Care 42(2):465–473
58. Brasil S, Frigieri G, Taccone FS et al (2023) Noninvasive intracranial pressure waveforms for estimation of intracranial hypertension and outcome prediction in acute brain-injured patients. J Clin Monit Comput 37(3):753–760
59. Brasil S, Cardim D, Caldas J et al (2024) Predicting short-term outcomes in brain-injured patients: a comprehensive approach with transcranial Doppler and intracranial compliance assessment. J Clin Monit Comput 38(6):1237–1247
60. Frigieri G, Gonçalves TL, Ocamoto GN, de Ap AR, de Padua BC, Cardim D (2025) Clinical Performance of the Brain4care System for Noninvasive Detection of Intracranial Hypertension. Neurocrit Care 43(2):628–635
61. Brasil S, Ben-Hur I, Cardim D, Czosnyka M, Paiva WS, Frigieri G (2025) Validation of a Noninvasive Approach for Cerebrospinal Compliance Monitoring. Neurocrit Care 43(1):186–194
62. de Moraes FM, Brasil S, Frigieri G, Robba C, Paiva W, Silva GS (2024) ICP wave morphology as a screening test to exclude intracranial hypertension in brain-injured patients: a non-invasive perspective. J Clin Monit Comput 38(4):773–782
63. Brasil S, Czosnyka M, Paiva WS, Frigieri G (2025) Exploring Cerebrospinal Compensatory Zones Using a Noninvasive Approach. Neurocrit Care 43(3):834–841
64. Frigieri G, Brasil S, Cardim D et al (2025) Machine learning approach for noninvasive intracranial pressure estimation using pulsatile cranial expansion waveforms. NPJ Digit Med 8(1):57
65. Ocamoto GN, da Silva LN, da Silva Rocha Tomaz C, et al (2024) Characterization of intracranial compliance in healthy subjects using a noninvasive method - results from a multicenter prospective observational study. J Clin Monit Comput 38(6): 1249–1261.
66. Karuta SCV, Folchini CM, Fachi MM et al (2024) Observational study of intracranial compliance analysis in neurologically healthy pediatric patients using a non-invasive device. Sci Rep 14(1):19482
67. Hassett CE, Uysal SP, Butler R, Moore NZ, Cardim D, Gomes JA (2023) Assessment of Cerebral Autoregulation Using Invasive and Noninvasive Methods of Intracranial Pressure Monitoring. Neurocrit Care 38(3):591–599
68. Frigieri G, Robba C, Machado FS, Gomes JA, Brasil S (2023) Application of non-invasive ICP waveform analysis in acute brain injury: Intracranial Compliance Scale. Intensive Care Med Exp 11(1):5
69. Brasil S, Solla DJF, Nogueira RC, Jacobsen Teixeira M, Malbouisson LMS, Paiva WS (2021) Intracranial Compliance Assessed by Intracranial Pressure Pulse Waveform. Brain Sci Jul 23; 11(8): 971.
70. Miller MT, Pasquale M, Kurek S et al (2004) Initial head computed tomographic scan characteristics have a linear relationship with initial intracranial pressure after trauma. J Trauma 56(5):967–972
71. Harder TJ, Leary OP, Yang Z et al (2023) Early Signs of Elevated Intracranial Pressure on Computed Tomography Correlate With Measured Intracranial Pressure in the Intensive Care Unit and Six-Month Outcome After Moderate to Severe Traumatic Brain Injury. J Neurotrauma 40(15–16):1603–1613
72. Alperin NJ, Lee SH, Loth F, Raksin PB, Lichtor T (2000) MR-Intracranial pressure (ICP): a method to measure intracranial elastance and pressure noninvasively by means of MR imaging: baboon and human study. Radiology 217(3):877–885
73. Kalantari H, Jaiswal R, Bruck I et al (2013) Correlation of optic nerve sheath diameter measurements by computed tomography and magnetic resonance imaging. Am J Emerg Med 31(11):1595–1597
74. Horton JC (2025) Idiopathic Intracranial Hypertension. N Engl J Med 393(14):1409–1419
75. Alkhachroum A, Appavu B, Egawa S et al (2022) Electroencephalogram in the intensive care unit: a focused look at acute brain injury. Intensive Care Med 48(10):1443–1462
76. Sheikh ZB, Maciel CB, Dhakar MB, Hirsch LJ, Gilmore EJ (2022) Non-epileptic Electroencephalographic Correlates of Episodic Increases in Intracranial Pressure. J Clin Neurophysiol 39(2):149–158
77. Bastani Viarsagh S, Agar A, Lawlor M, Fraser C, Golzan M (2024) Non-invasive assessment of intracranial pressure through the eyes: current developments, limitations, and future directions. Front Neurol 15:1442821
78. Liu X, Kale AU, Capewell N et al (2019) Optical coherence tomography (OCT) in unconscious and systemically unwell patients using a mobile OCT device: a pilot study. BMJ Open 9(11):e030882
79. Robba C, Bacigaluppi S, Cardim D, Donnelly J, Bertuccio A, Czosnyka M (2016) Non-invasive assessment of intracranial pressure. Acta Neurol Scand 134(1):4–21
80. Bruce BB (2014) Noninvasive assessment of cerebrospinal fluid pressure. J Neuroophthalmol 34(3):288–294
81. Reid A, Marchbanks RJ, Burge DM et al (1990) The relationship between intracranial pressure and tympanic membrane displacement. Br J Audiol 24(2):123–129
82. Uryga A, Kazimierska A, Popek M et al (2023) Applying video motion magnification to reveal spontaneous tympanic membrane displacement as an indirect measure of intracranial pressure in patients with brain pathologies. Acta Neurochir (Wien) 165(8):2227–2235
83. Ragauskas A, Matijosaitis V, Zakelis R et al (2012) Clinical assessment of noninvasive intracranial pressure absolute value measurement method. Neurology 78(21):1684–1691
84. Chesnut RM, Temkin N, Carney N et al (2012) A trial of intracranial-pressure monitoring in traumatic brain injury. N Engl J Med 367(26):2471–2481
85. Robba C, Busl KM, Claassen J, et al (2024) Contemporary management of aneurysmal subarachnoid haemorrhage. An update for the intensivist. Intensive Care Med 50(5): 646–64.
86. Dallagiacoma S, Robba C, Graziano F, et al (2022) SYNAPSE-ICU Investigators. Intracranial Pressure Monitoring in Patients With Spontaneous Intracerebral Hemorrhage: Insights From the SYNAPSE-ICU Study. Neurology 99(2): e98-e108.
87. Robba C, van Dijk EJ, van der Jagt M (2022) Acute ischaemic stroke and its challenges for the intensivist. Eur Heart J Acute Cardiovasc Care 11(3):258–268
88. Hollingworth M, Jamjoom AAB, Bulters D, Patel HC (2019) How is vasospasm screening using transcranial Doppler associated with delayed cerebral ischemia and outcomes in aneurysmal subarachnoid hemorrhage? Acta Neurochir (Wien) 161(2):385–392
89. Tasker RC, Menon DK (2016) Critical Care and the Brain. JAMA 315(8):749–750
90. Mrozek S, Gobin J, Constantin JM, Fourcade O, Geeraerts T (2020) Cross-talk between brain, lung and heart in critical care. Anaesth Crit Care Pain Med 39(4):519–530
91. Laver S, Farrow C, Turner D, Nolan J (2004) Mode of death after admission to an intensive care unit following cardiac arrest. Intensive Care Med 30(11):2126–2128
92. Lemiale V, Dumas F, Mongardon N et al (2013) Intensive care unit mortality after cardiac arrest: the relative contribution of shock and brain injury in a large cohort. Intensive Care Med 39(11):1972–1980
93. Sandroni C, Cronberg T, Sekhon M (2021) Brain injury after cardiac arrest: pathophysiology, treatment, and prognosis. Intensive Care Med 47(12):1393–1414
94. Albaiceta GM, Brochard L, Dos Santos CC et al (2021) The central nervous system during lung injury and mechanical ventilation: a narrative review. Br J Anaesth 127(4):648–659
95. Villalba N, Ma Y, Gahan SA et al (2023) Lung infection by Pseudomonas aeruginosa induces neuroinflammation and blood-brain barrier dysfunction in mice. J Neuroinflammation 20(1):127

96. Hoiland RL, Bain AR, Rieger MG, Bailey DM, Ainslie PN (2016) Hypoxemia, oxygen content, and the regulation of cerebral blood flow. Am J Physiol Regul Integr Comp Physiol 310(5):R398-413
97. Mascia L, Grasso S, Fiore T, Bruno F, Berardino M, Ducati A (2005) Cerebro-pulmonary interactions during the application of low levels of positive end-expiratory pressure. Intensive Care Med 31(3):373–379
98. Iavarone IG, Rocco PRM, Grieco DL et al (2025) Pathophysiology and clinical applications of PEEP in acute brain injury. Intensive Care Med 51(11):2104–2116
99. Sanfilippo F, Uryga A, Ball L et al (2024) The Effect of Recruitment Maneuvers on Cerebrovascular Dynamics and Right Ventricular Function in Patients with Acute Brain Injury: A Single-Center Prospective Study. Neurocrit Care 41(1):38–48
100. Rama Rao KV, Jayakumar AR, Norenberg MD (2014) Brain edema in acute liver failure: mechanisms and concepts. Metab Brain Dis 29(4):927–936
101. Gilmore EJ, Gaspard N, Choi HA et al (2015) Acute brain failure in severe sepsis: a prospective study in the medical intensive care unit utilizing continuous EEG monitoring. Intensive Care Med 41(4):686–694
102. Hoedemaekers CW, Ainslie PN, Hinssen S et al (2017) Low cerebral blood flow after cardiac arrest is not associated with anaerobic cerebral metabolism. Resuscitation 120:45–50
103. Lemiale V, Huet O, Vigué B et al (2008) Changes in cerebral blood flow and oxygen extraction during post-resuscitation syndrome. Resuscitation 76(1):17–24
104. Rafi S, Tadie JM, Gacouin A et al (2019) Doppler sonography of cerebral blood flow for early prognostication after out-of-hospital cardiac arrest: DOTAC study. Resuscitation 141:188–194
105. Cardim D, Griesdale DE, Ainslie PN et al (2019) A comparison of non-invasive versus invasive measures of intracranial pressure in hypoxic ischaemic brain injury after cardiac arrest. Resuscitation 137:221–228
106. Tamura T, Namiki J, Sugawara Y et al (2018) Quantitative assessment of pupillary light reflex for early prediction of outcomes after out-of-hospital cardiac arrest: A multicentre prospective observational study. Resuscitation 131:108–113
107. Riker RR, Sawyer ME, Fischman VG et al (2020) Neurological Pupil Index and Pupillary Light Reflex by Pupillometry Predict Outcome Early After Cardiac Arrest. Neurocrit Care 32(1):152–161
108. Suys T, Bouzat P, Marques-Vidal P et al (2014) Automated quantitative pupillometry for the prognostication of coma after cardiac arrest. Neurocrit Care 21(2):300–308
109. Heimburger D, Durand M, Gaide-Chevronnay L et al (2016) Quantitative pupillometry and transcranial Doppler measurements in patients treated with hypothermia after cardiac arrest. Resuscitation 103:88–93
110. Oddo M, Sandroni C, Citerio G et al (2018) Quantitative versus standard pupillary light reflex for early prognostication in comatose cardiac arrest patients: an international prospective multicenter double-blinded study. Intensive Care Med 44(12):2102–2111
111. MacDonald AJ, Speiser JL, Ganger DR et al (2021) Clinical and Neurologic Outcomes in Acetaminophen-Induced Acute Liver Failure: A 21-Year Multicenter Cohort Study. Clin Gastroenterol Hepatol 19(12):2615–2625
112. Escorsell A, Mas A, de la Mata M; Spanish Group for the Study of Acute Liver Failure (2007) Acute liver failure in Spain: analysis of 267 cases. Liver Transpl 13(10):1389–1395
113. Rajajee V, Williamson CA, Fontana RJ, Courey AJ, Patil PG (2018) Noninvasive Intracranial Pressure Assessment in Acute Liver Failure. Neurocrit Care 29(2):280–290
114. Helmke K, Burdelski M, Hansen HC (2000) Detection and monitoring of intracranial pressure dysregulation in liver failure by ultrasound. Transplantation 70(2):392–395
115. Vijay P, Lal BB, Sood V, Khanna R, Patidar Y, Alam S (2021) Dynamic Optic Nerve Sheath Diameter (ONSD) guided management of raised intracranial pressure in pediatric acute liver failure. Hepatol Int 15(2):502–509
116. Schuurman PR, Albrecht KW (1999) Intraoperative changes of transcranial Doppler velocity: relation to arterial oxygen content and whole-blood viscosity. Ultrasound Med Biol 25(1):151–154
117. Cigada M, Marzorati S, Tredici S, Iapichino G (2000) Cerebral CO2 vasoreactivity evaluation by transcranial Doppler ultrasound technique: a standardized methodology. Intensive Care Med 26(6):729–732
118. Kirkham FJ, Padayachee TS, Parsons S, Seargeant LS, House FR, Gosling RG (1986) Transcranial measurement of blood velocities in the basal cerebral arteries using pulsed Doppler ultrasound: velocity as an index of flow. Ultrasound Med Biol 12(1):15–21
119. Eng C, Lam AM, Mayberg TS, Lee C, Mathisen T (1992) The influence of propofol with and without nitrous oxide on cerebral blood flow velocity and CO2 reactivity in humans. Anesthesiology 77(5):872–879
120. Klinzing S, Stretti F, Pagnamenta A, Bèchir M, Brandi G (2021) Transcranial color-coded duplex sonography assessment of cerebrovascular reactivity to carbon dioxide: an interventional study. BMC Neurol 21(1):305
121. Schramm P, Closhen D, Felkel M et al (2013) Influence of PEEP on cerebral blood flow and cerebrovascular autoregulation in patients with acute respiratory distress syndrome. J Neurosurg Anesthesiol 25(2):162–167
122. Muench E, Bauhuf C, Roth H et al (2005) Effects of positive end-expiratory pressure on regional cerebral blood flow, intracranial pressure, and brain tissue oxygenation. Crit Care Med 33(10):2367–2372
123. Boone MD, Jinadasa SP, Mueller A et al (2017) The Effect of Positive End-Expiratory Pressure on Intracranial Pressure and Cerebral Hemodynamics. Neurocrit Care 26(2):174–181
124. Chen H, Chen K, Xu JQ, Zhang YR, Yu RG, Zhou JX (2018) Intracranial pressure responsiveness to positive end-expiratory pressure is influenced by chest wall elastance: a physiological study in patients with aneurysmal subarachnoid hemorrhage. BMC Neurol 18(1):124
125. Brunetti DJ, Leonardis F, Frisardi F et al (2025) Effects of "Head Up" Prone Position on Transcranial Color Doppler-Based Estimators of Intracranial Pressure in Moderate to Severe Acute Respiratory Distress Syndrome Without Brain Injury: A Cross-Over, Longitudinal. Physiological Study Neurocrit Care 43(2):446–457
126. Elmaleh Y, Yavchitz A, Léguillier T, Squara PA, Palpacuer C, Grégoire C (2024) Feasibility of Prone Positioning for Brain-injured Patients with Severe Acute Respiratory Distress Syndrome: A Systematic Review and Pilot Study (ProBrain). Anesthesiology 140(3):495–512
127. Wahlster S, Town JA, Robba C (2025) Head up, face down-a practical framework for proning brain-injured patients with ARDS. Intensive Care Med 51(10):1909–1912
128. Cho SM, Hwang J, Chiarini G, et al. (2024) Neurological monitoring and management for adult extracorporeal membrane oxygenation patients: Extracorporeal Life Support Organization consensus guidelines. Crit Care Sep 6; 28(1):296.
129. Crippa IA, Vincent JL, Zama Cavicchi F et al (2024) Estimated Cerebral Perfusion Pressure and Intracranial Pressure in Septic Patients. Neurocrit Care 40(2):577–586
130. Mowafy SMS, Bauiomy H, Kohaf NA, Abd Ellatif SE (2025) The Role of Ultrasonographic Assessment of Optic Nerve Sheath Diameter in Prediction of Sepsis-Associated Encephalopathy: Prospective Observational Study. Neurocrit Care 43(1):308–317
131. Crippa IA, Subirà C, Vincent JL et al (2018) Impaired cerebral autoregulation is associated with brain dysfunction in patients with sepsis. Crit Care 22(1):327
132. Patel S, Maria-Rios J, Parikh A, Okorie ON (2023) Diagnosis and management of elevated intracranial pressure in the emergency department. Int J Emerg Med 16(1):72
133. Kalmar AF, Van Aken J, Caemaert J, Mortier EP, Struys MM (2005) Value of Cushing reflex as warning sign for brain ischaemia during neuroendoscopy. Br J Anaesth 94(6):791–799
134. Ter Avest E, Taylor S, Wilson M, Lyon RL (2021) Prehospital clinical signs are a poor predictor of raised intracranial pressure following traumatic brain injury. Emerg Med J 38(1):21–26
135. Yumoto T, Mitsuhashi T, Yamakawa Y et al (2016) Impact of Cushing's sign in the prehospital setting on predicting the need for immediate neurosurgical intervention in trauma patients: a nationwide retrospective observational study. Scand J Trauma Resusc Emerg Med 24(1):147
136. Robba C, Goffi A, Geeraerts T et al (2019) Brain ultrasonography: methodology, basic and advanced principles and clinical applications. A narrative review Intensive Care Med 45(7):913–927

137. Deana C, Biasucci DG, Aspide R et al (2025) Non-invasive intracranial pressure assessment in adult critically ill patients: A narrative review on current approaches and future perspectives. J Clin Anesth 106:111977
138. Teasdale G, Jennett B (1974) Assessment of coma and impaired consciousness. A practical scale Lancet 2(7872):81–84
139. Sharshar T, Citerio G, Andrews PJ, et al (2014) Neurological examination of critically ill patients: a pragmatic approach. Report of an ESICM expert panel. Intensive Care Med 40(4): 484–95.
140. Schweitzer AD, Niogi SN, Whitlow CT, Tsiouris AJ (2019) Traumatic Brain Injury: Imaging Patterns and Complications. Radiographics 39(6):1571–1595
141. Maas AIR, Menon DK, Manley GT et al (2022) Traumatic brain injury: progress and challenges in prevention, clinical care, and research. Lancet Neurol 21(11):1004–1060
142. Rubiano AM, Griswold DP, Jibaja M, Rabinstein AA, Godoy DA (2021) Management of severe traumatic brain injury in regions with limited resources. Brain Inj 35(11):1317–1325
143. Godoy DA, Rabinstein AA (2022) How to manage traumatic brain injury without invasive monitoring? Curr Opin Crit Care 28(2):111–122
144. Chesnut RM, Temkin N, Videtta W et al (2020) Consensus-Based Management Protocol (CREVICE Protocol) for the Treatment of Severe Traumatic Brain Injury Based on Imaging and Clinical Examination for Use When Intracranial Pressure Monitoring Is Not Employed. J Neurotrauma 37(11):1291–1299
145. Chesnut RM, Temkin N, Videtta W et al (2023) Testing the Impact of Protocolized Care of Patients With Severe Traumatic Brain Injury Without Intracranial Pressure Monitoring: The Imaging and Clinical Examination Protocol. Neurosurgery 92(3):472–480
146. Chesnut RM, Temkin N, Videtta W, et al (2023) The Roles of Protocols and Protocolization in Improving Outcome From Severe Traumatic Brain Injury. Neurosurgery. Epub ahead of print.
147. Rubiano AM, Vera DS, Montenegro JH et al (2020) Recommendations of the Colombian Consensus Committee for the Management of Traumatic Brain Injury in Prehospital, Emergency Department, Surgery, and Intensive Care (Beyond One Option for Treatment of Traumatic Brain Injury: A Stratified Protocol [BOOTStraP]). J Neurosci Rural Pract 11(1):7–22
148. Picetti E, Antonini MV, Lucchetti MC et al (2013) Intra-hospital transport of brain-injured patients: a prospective, observational study. Neurocrit Care 18(3):298–304
149. Godoy DA, Pérez-Bárcena J, Delgado-Moya FP, Barea-Mendoza JA, Llompart-Pou JA (2025) Noninvasive bedside neuromonitoring in acute brain injury. A narrative review. Med Intensiva (Engl Ed). Epub ahead of print.
150. Güiza F, Depreitere B, Piper I et al (2015) Visualizing the pressure and time burden of intracranial hypertension in adult and paediatric traumatic brain injury. Intensive Care Med 41(6):1067–1076
151. Puffer RC, Rubiano AM, Oczkowski S et al (2024) Methodology for the Formulation of the Guidelines for the Management of Moderate to Severe Traumatic Brain Injury in Austere and Combat Environments. Neurosurg Pract 5(3):e00104
152. Dengler B, McCafferty R, Neal C et al (2025) A Joint Trauma System Clinical Practice Guideline: Traumatic Brain Injury Management and Basic Neurosurgery in the Deployed Environment. Mil Med 190(1–2):124–134
153. Bazarian JJ, Zetterberg H, Buki A et al (2025) Blood-Based Biomarkers for Improved Characterization of Traumatic Brain Injury: Recommendations from the 2024 National Institute for Neurological Disorders and Stroke Traumatic Brain Injury Classification and Nomenclature Initiative Blood-Based Biomarkers Working Group. J Neurotrauma 42(13–14):1065–1085
154. Peters J, Van Wageningen B, Hoogerwerf N, Tan E (2017) Near-Infrared Spectroscopy: A Promising Prehospital Tool for Management of Traumatic Brain Injury. Prehosp Disaster Med 32(4):414–418
155. Joubert C, Sellier A, Beucler N et al (2023) Application of a Near-infrared Spectroscope by an Extreme Forward Medical Team for the Triage of Casualties With Traumatic Brain Injury. Mil Med 188(3–4):e572–e578